

The American College of Radiology, with more than 30,000 members, is the principal organization of radiologists, radiation oncologists, and clinical medical physicists in the United States. The College is a nonprofit professional society whose primary purposes are to advance the science of radiology, improve radiologic services to the patient, study the socioeconomic aspects of the practice of radiology, and encourage continuing education for radiologists, radiation oncologists, medical physicists, and persons practicing in allied professional fields.

The American College of Radiology will periodically define new practice guidelines and technical standards for radiologic practice to help advance the science of radiology and to improve the quality of service to patients throughout the United States. Existing practice guidelines and technical standards will be reviewed for revision or renewal, as appropriate, on their fifth anniversary or sooner, if indicated.

Each practice guideline and technical standard, representing a policy statement by the College, has undergone a thorough consensus process in which it has been subjected to extensive review, requiring the approval of the Commission on Quality and Safety as well as the ACR Board of Chancellors, the ACR Council Steering Committee, and the ACR Council. The practice guidelines and technical standards recognize that the safe and effective use of diagnostic and therapeutic radiology requires specific training, skills, and techniques, as described in each document. Reproduction or modification of the published practice guideline and technical standard by those entities not providing these services is not authorized.

2004 (Res. 7)
Amended 2006 (Res. 17,35)
Effective 10/01/04

ACR PRACTICE GUIDELINE FOR THE PERFORMANCE OF RADIOGRAPHY FOR SCOLIOSIS IN CHILDREN

PREAMBLE

These guidelines are an educational tool designed to assist practitioners in providing appropriate radiologic care for patients. They are not inflexible rules or requirements of practice and are not intended, nor should they be used, to establish a legal standard of care. For these reasons and those set forth below, the American College of Radiology cautions against the use of these guidelines in litigation in which the clinical decisions of a practitioner are called into question.

The ultimate judgment regarding the propriety of any specific procedure or course of action must be made by the physician or medical physicist in light of all the circumstances presented. Thus, an approach that differs from the guidelines, standing alone, does not necessarily imply that the approach was below the standard of care. To the contrary, a conscientious practitioner may responsibly adopt a course of action different from that set forth in the guidelines when, in the reasonable judgment of the practitioner, such course of action is indicated by the condition of the patient, limitations on available resources, or advances in knowledge or technology subsequent to publication of the guidelines. However, a practitioner who employs an approach substantially different from these guidelines is advised to document in the patient record information sufficient to explain the approach taken.

The practice of medicine involves not only the science, but also the art of dealing with the prevention, diagnosis, alleviation, and treatment of disease. The variety and

complexity of human conditions make it impossible to always reach the most appropriate diagnosis or to predict with certainty a particular response to treatment. Therefore, it should be recognized that adherence to these guidelines will not assure an accurate diagnosis or a successful outcome. All that should be expected is that the practitioner will follow a reasonable course of action based on current knowledge, available resources, and the needs of the patient to deliver effective and safe medical care. The sole purpose of these guidelines is to assist practitioners in achieving this objective.

I. INTRODUCTION

Scoliosis is a lateral curvature of the vertebral column. Radiography is a proven and useful procedure to confirm the presence, location, and degree of spinal curvature. This guideline outlines the principles for performing high-quality radiography of the spine for scoliosis in children.

Radiography for scoliosis in children should be performed only for a valid medical reason and with the minimum radiation dose necessary to achieve an optimal study. Additional views or specialized examinations may be required. While it is not possible to detect all scoliosis abnormalities, adherence to the following guideline will maximize the probability of their detection.

All radiographic examinations should be performed in accordance with the [ACR Practice Guideline for General Radiography](#).

II. INDICATIONS

Indications for radiography of the spine for scoliosis include, but are not limited to, the following:

1. Alterations in normal spinal alignment on physical examination.
2. Evaluation of spinal curvature progression.
3. Follow-up of treatment (orthotic or surgical).
4. Parent or sibling with scoliosis.

All imaging facilities should have policies and procedures to reasonably attempt to identify pregnant patients prior to the performance of any examination involving ionizing radiation. If the patient is known to be pregnant, the potential radiation risks to the fetus and clinical benefits of the procedure should be considered before proceeding with the study. (1995, 2005 - ACR Resolution 1a)

III. QUALIFICATIONS AND RESPONSIBILITIES OF PERSONNEL

See the [ACR Practice Guideline for General Radiography](#).

IV. SPECIFICATIONS OF EXAMINATION

The written or electronic request for a radiograph for a scoliosis evaluation should provide sufficient information to demonstrate the medical necessity of the examination and allow for its proper performance and interpretation.

Documentation that satisfies medical necessity includes 1) signs and symptoms and/or 2) relevant history (including known diagnoses). Additional information regarding the specific reason for the examination or a provisional diagnosis would be helpful and may at times be needed to allow for the proper performance and interpretation of the examination.

The request for the examination must be originated by a physician or other appropriately licensed health care provider. The accompanying clinical information should be provided by a physician or other appropriately licensed health care provider familiar with the patient's clinical problem or question and consistent with the state scope of practice requirements. (2006 - ACR Resolution 35)

A. Scoliosis Survey

The preferred practice consists of posteroanterior (PA) radiography of the spine obtained in the upright position.

The number of images required for complete evaluation of scoliosis varies with the clinical indications. When possible, a single upright PA image of the thoracolumbar spine should be obtained at a minimum source-to-receptor distance of 6 feet and an image size of either 14" x 17" or 14" x 36". The patient should stand or sit before a vertical

grid. When standing, the knees are placed together in full extension. PA positioning of the patient decreases radiation dose to the thyroid and breast. The field of view should extend from the edge of the mandible to the top of the greater trochanter. Methods to decrease radiation exposure may include lead-acrylic filters, breast shields (especially for anteroposterior (AP) examinations), increased beam filtration, high-speed films and screens, and beam collimation. Gonadal shielding can be used when the area of curvature does not include the sacrum.

For patients unable to stand or sit before a vertical grid, an AP image may be obtained. A shorter source to receptor distance can be used.

B. Imaging for Patients Being Assessed or Clinically Treated for Scoliosis

For patients who are being assessed or clinically treated for scoliosis, additional images may include:

1. Right and left lateral bending images. Preoperative studies may often include bilateral bending images in the frontal projection of both the thoracic and lumbar spine curves.
2. A lateral vertical beam image.
3. PA examination of the left wrist and hand for bone age.

V. DOCUMENTATION

A. It is important that new images be compared with prior examinations and/or other pertinent studies that may be available.

B. Reporting should be in accordance with the [ACR Practice Guideline for Communication of Diagnostic Imaging Findings](#).

1. Radiographic analysis of scoliosis should identify presence, direction, location, and/or apex of the curvature. Evaluation includes a description of any vertebral or paraspinal abnormalities and the presence of pelvic inclination (tilt). Note should be made of the presence of a brace or a shoelift. The degree of scoliosis, kyphosis/lordosis, and/or axial rotation may be measured and quantified using established techniques. If the study is a follow-up examination, any progression of the curvature(s) should be described.
2. Determination of skeletal maturity is important to the assessment of scoliosis, as mild to moderate scoliotic curves do not progress after growth cessation. Skeletal maturity may be evaluated by analyzing the development of the iliac crest apophysis, as described by Risser, or

by analyzing images of the hands and wrists according to the method of Greulich and Pyle.

VI. EQUIPMENT SPECIFICATIONS

Radiographic images shall be exposed only with equipment having a beam-limiting device that provides rectangular collimators.

A wall-mounted device must be available to accommodate a 14" x 17" and/or a 14" x 36" receptor device.

VII. RADIATION SAFETY IN IMAGING

Radiologists, medical physicists, radiologic technologists, and all supervising physicians have a responsibility to minimize radiation dose to individual patients, staff, and to society as a whole, while maintaining the necessary diagnostic image quality. This is the concept "As Low As Reasonably Achievable (ALARA)".

Facilities, in consultation with the medical physicist, should have in place and should adhere to policies and procedures, in accordance with ALARA, to vary examination protocols to take into account patient body habitus, such as height and/or weight, body mass index or lateral width. The dose reduction devices that are available on imaging equipment should be active or manual techniques should be used to moderate the exposure while maintaining the necessary diagnostic image quality. Patient radiation doses should be periodically measured by a medical physicist in accordance with the appropriate ACR Technical Standard. (2006 - ACR Resolution 17)

VIII. QUALITY CONTROL AND IMPROVEMENT, SAFETY, INFECTION CONTROL, AND PATIENT EDUCATION CONCERNS

Policies and procedures related to quality, patient education, infection control, and safety should be developed and implemented in accordance with the ACR Policy on Quality Control and Improvement, Safety, Infection Control, and Patient Education Concerns appearing elsewhere in the ACR Practice Guidelines and Technical Standards book.

Equipment performance monitoring should be in accordance with the [ACR Technical Standard for Diagnostic Medical Physics Performance Monitoring of Radiographic and Fluoroscopic Equipment](#).

ACKNOWLEDGEMENTS

This guideline was developed according to the process described in the ACR Practice Guidelines and Technical Standards book by the Guidelines and Standards Committee of the Commission on General and Pediatric Radiology.

Principal Drafter: Eric N. Faerber, MD

Drafters: Michael C. Beachley, MD
Kimberly E. Applegate, MD
Edward Weinberger, MD

Guidelines and Standards Committee

Michael C. Beachley, MD, Chair
Kimberly E. Applegate, MD
Richard A. Carlson, MD
Kevin M. Cawley, MD
Ronald E. Cordell, MD
Eric N. Faerber, MD
Edmund A. Franken, Jr., MD
Bob W. Gayler, MD
Sam Kottamasu, MD
Arvin E. Robinson, MD
Diane C. Stollo, MD
Edward Weinberger, MD

J. Bruce Hauser, MD, Chair, Commission
David C. Kushner, MD, Co-Chair, CSC Subcommittee
Paul A. Larson, MD, Co-Chair, CSC Subcommittee

REFERENCES

1. Asher MA. Scoliosis evaluation. *Orthop Clin North Am* 1988;19:805-814.
2. Barsanti CM, deBari A, Covino BM. The torsion meter: a critical review. *J Pediatr Orthop* 1990;10:527-531.
3. Biondi J, Weiner DS, Bethem D, et al. Correlation of Risser sign and bone age determination in adolescent idiopathic scoliosis. *J Pediatr Orthop* 1985;5:697-701.
4. Butler PF, Thomas AW, Thompson WE, et al. Simple methods to reduce patient exposure during scoliosis radiography. *Radiol Technol* 1986;57:411-417.
5. Cobb JR. Outline for the study of scoliosis. *AAOS Instructional Course Lectures* 1948;5:261-275.
6. De Smet AA, Fritz SL, Asher MA. A method for minimizing the radiation exposure from scoliosis radiographs. *J Bone Joint Surg Am* 1981;63:156-61.
7. De Smet AA. *Radiology of Spinal Curvature*. St Louis, Mo: CW Mosby Company; 1985:39-43.
8. Gray JE, Hoffman AD, Peterson HA. Reduction of radiation exposure during radiography for scoliosis. *J Bone Joint Surg Am* 1983;65:5-12.

9. Gundry CR, Heithoff KB. Imaging evaluation of patients with spinal deformity. *Orthop Clin North Am* 1994;25:247-264.
10. Greulich WW, Pyle SI. *Radiographic Atlas of Skeletal Development of the Hand and Wrist*. 2nd edition. Stanford, Calif: Stanford University Press; 1959.
11. Hansen J, Jurik AG, Fiirgaard B, et al. Optimisation of scoliosis examinations in children. *Pediatric Radiol* 2003;33:752-765.
12. Levy AR, Goldberg MS, Mayo NE, et al. Reducing the lifetime risk of cancer from spinal radiographs among people with adolescent idiopathic scoliosis. *Spine* 1996;21:1540-1547.
13. Levy AR, Goldberg MS, Hanley JA, et al. Projecting the lifetime risk of cancer from exposure to diagnostic ionizing radiation for adolescent idiopathic scoliosis. *Health Phys* 1994;66:621-633.
14. Lonstein JE. Patient evaluation. In: Lonstein JE, Bradford DS, Winter RB, et al. *Moe's Textbook of Scoliosis and Other Spinal Deformities*. 3rd edition. Philadelphia, Pa: WB Saunders Co; 1995:68-75.
15. McAlister WH, Shackelford GD. Measurement of spinal curvatures. *Radiol Clin North Am* 1975;13:113-121.
16. Nash CL Jr., Moe JH. A study of vertebral rotation. *J Bone Joint Surg Am* 1969;51:223-229.
17. Oestreich AE, Young LW, Poussaint TY. Scoliosis circa 2000: radiologic imaging perspective: diagnosis and pretreatment evaluation. *Skeletal Radiol* 1998;27:591-605.
18. Perdriolle R. *La Scoliose: Son Etude Tridimensionnelle*. Paris Maloine SA, 1979:16-17.
19. Risser JC. Scoliosis: past and present. *J Bone Joint Surg* 1964;46:167-199.
20. Stokes IA. Three-dimensional terminology of spinal deformity. A report presented to the Scoliosis Research Society by the Scoliosis Research Society working group on 3-D terminology of spinal deformity. *Spine* 1994;15:236-248.
21. Stokes IA. *Terminology Committee and Working Group on Spinal Classification: Revised Glossary of Terms*. Available at: <http://www.uvm.edu/istokes/srs/srsnomen.htm>. Accessed December 9, 2003.
22. Wright N. Imaging in scoliosis. *Arch Dis Child* 2000;82:38-40.

endplate lines. The angle subtended by these lines is the angle of curvature.

Scoliosis Research Committee (SRS) Terminology – Selected Terms:

Apical vertebra (apex) – in a curve, the vertebra most deviated laterally from the vertical axis that passes through the center of the sacrum.

Compensatory curve – a minor curve above or below a major curve that may or may not be structural.

Hyperkyphosis – a kyphosis greater than the normal range.

Hyperlordosis – a lordosis greater than the normal range.

Lumbar scoliosis – a scoliosis that has its apex at a point between the L1-L2 disc space and the L4-L5 disc space.

Pelvic inclination – deviation of the pelvic outlet from the vertical, measured as an angle between the line from the top of the sacrum to the top of the pubis, and a horizontal line perpendicular to the lateral edge of the standing radiograph.

Thoracic scoliosis – a scoliosis that has its apex at a point between the T2 vertebral body and the T11-T12 disc.

Thoracolumbar scoliosis – a scoliosis with its apex at T12, L1, or the intervening T12-L1 disc.

Vertebral axial rotation – transverse plane angulation of a vertebra: one method of measurement is with the Perdriolle technique (in degrees).


APPENDIX

Glossary

Cobb measurement of angle – The “end vertebrae” are identified. The end vertebrae are the vertebrae tilted maximally toward the concavity of the curve. Parallel lines are drawn along with superior endplate of the upper end vertebra and the inferior endplate of the lower end vertebra or through the pedicles if the endplates are indistinct. Lines are constructed perpendicular to these

Measurement of Rotation


Nash and Moe Method:

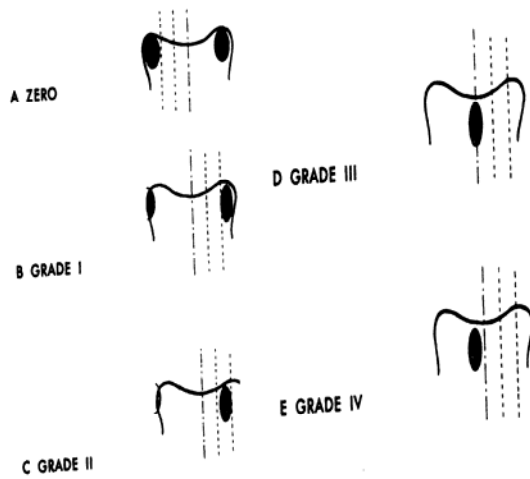

- A. Zero rotation. The pedicles are equidistant from the lateral margins of the vertebral body.
- B. Grade I rotation. The pedicle on the convexity has moved from the edge of the vertebral body.
- C. Grade II rotation. Rotation intermediate between Grade I and Grade III.
- D. Grade III rotation. The pedicle is close to the center of the vertebral body.
- E. Grade IV rotation. The pedicle is past the center of the vertebral body.


From: Nash C, Moe J. A study of vertebral rotation. *J Bone Joint Surg* 1969; 51:223–229.

Perdriolle Method:

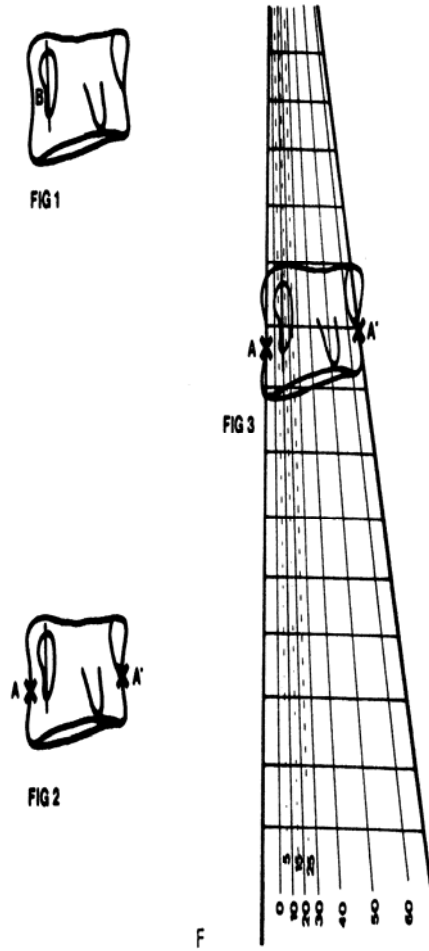

The measurement of vertebral rotation is made from the pedicle situated at the convexity of the apical vertebra under consideration. Fig. 1: mark the greatest diameter of the pedicle (B). Fig. 2: mark a reference at the waist of each lateral border of the vertebra (A and A'). Fig 3: superimpose the torsionmeter on the vertebra so that the edges of the rule are at the sides of the vertebral body. The amount of rotation of the pedicle line is read from the rotation scale, 10 degrees in this example. (Redrawn from Perdriolle R: *La Scoliose*, Maloine, SA editeur, Paris, 1979.)

Risser grading of iliac apophysis maturity:

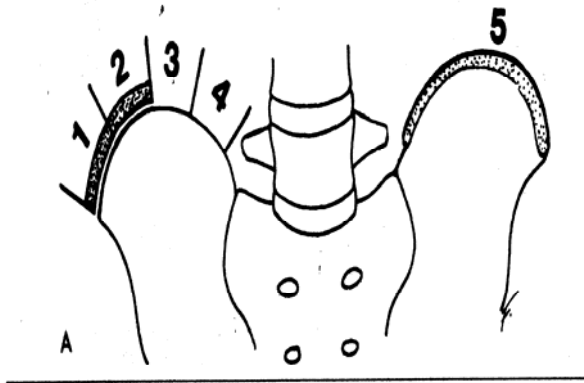

Kyphosis and Lordosis: Measurement and Normal Ranges:

The recommended measurement of thoracic kyphosis from a lateral radiograph is the angle between the superior endplate of the highest measurable thoracic vertebra, usually T2 or T3, and the inferior endplate of T12.

The recommended measurement of lumbar lordosis from a lateral radiograph is the angle between the superior endplate of L1 and the superior endplate of S1.

Normal range for thoracic kyphosis: 20-50 degrees

Normal range for lumbar lordosis: 20-60 degrees